pierre cardin
PARIS

IPL LAZER EPİLASYON

PC-L10001

pierre cardin
PARIS

CE RoHS

İthalatçı Firma Bilgileri:
Teknokta İç Dış Tic. Ltd. Şti.
Adres: Küçükbakkalköy Mh. Kayışdağı Cd. Ayşe Hatun Çeşme Sk. No:9 Kat:-1,0,1,2 PK: 34775 Ataşehir / İstanbul
Telefon: +90 216 600 20 00 | Fax: +90 216 576 38 78

1.Güvenlik Talimatları

Yoğun Atımlı Işık (IPL) Sistemini ilk kez kullanmadan önce lütfen kullanım kılavuzunu dikkatlice okuyun.

⚠ **UYARI**

- Bu ürün oyuncak değildir, çocukların ulaşamayacağı yerlerde saklayın.
- Lütfen kullanmaya başlamadan önce cihazı doğrulayın. Herhangi bir hasar varsa KULLANMAYIN.
- Cihazı ve güç adaptörünü kuru tutun.
- Cihazın çalışma voltajının, güç kaynağının nominal voltajına uygun olduğundan emin olun.
- Cihazı kullanırken her zaman gözlük taktığınızdan emin olun.

⚠ **DİKKAT**

Yoğun Atımlı Işık (IPL) Sistemi elektrikli bir cihazdır. Bu nedenle, güvenliğe özel dikkat gösterilerek kullanılmalıdır. Lütfen kullanmadan önce tüm uyarıları ve ikazları okuyun ve cihazı kullanırken bunlara kesinlikle uyun.

Kontrendikasyonlar:

Aşağıdaki kişiler bu cihazı kullanmamalıdır:

- Hamileler veya emziren ya da adet dönemindeki kadınlar ile çocuklar.
- Cildiniz ışığa karşı hassas ve döküntü veya alerjik reaksiyon geliştirmeye yatkın ise.
- V ve VI cilt tipine sahipseniz (nadiren veya hiç güneş yanığı olmuyor, çok koyu bronzlaşıyorsanız). Bu durumda, hiperpigmentasyon ve hipopigmentasyon, şiddetli kızarıklık veya yanık gibi cilt reaksiyonları geliştirme riskiniz yüksektir.
- Daha önceden cilt hastalığı geçirmiş veya halen ciltle ilgili hastalıklar nedeniyle tedavi görmekte olan kişiler.
- Cihazı kullanmak istediklerí bölgelerde prekanseröz lezyonlar veya çoklu atipik doğum lekeleri (benler) olan kişiler.
- Uygulamak istediğiniz bölgede enfeksiyon, yanık, egzama, kıl kökü iltihabı, çizik, açık yara, uçuk, kesik veya kan oturması varsa.
- Kolajen bozukluğu, keloid yara izi oluşumu veya yaraların iyileşmesinde zorluk öyküsü olan kişiler.
- Varisli damar gibi damar hastalıkları öyküsü olan kişiler.
- Diyabet, lupus eritematozus, porfiri, konjestif kalp hastalığı ve kanama bozukluğu olan kişiler.
- Bağışıklık sistemini baskılayıcı hastalık öyküsü olan kişiler (HIV enfeksiyonu ve AIDS dahil).
- Radyoterapi veya kemoterapi alıyorsanız veya son birkaç ay içinde aldıysanız.

⚠ **UYARI**

Bu cihazı aşağıdaki alanlarda KULLANMAYIN:

- Hiperpigmentasyon veya hipopigmentasyon, yoğun kızarıklık veya yanık olan bölgelerde.
- Ameliyat olduğunuz bölgelerde.
- Göz yaralanmasını önlemek için göz ve kaş çevresinde.
- Meme uçlarında, meme ucu çevresinde, vajina iç dudaklarında, vajinada, anüste, burun deliğinin içinde ve kulaklarda. Erkekler bu cihazı testis torbası ve yüz üzerinde kullanmamalıdır.
- Silikon implantlar, kalp pilleri, deri altı enjeksiyon kanalı (insülin dağıtıcıları gibi), vücut piercingleri yakınında. Herhangi bir yapay yüzeyden uzak durulmalıdır.
- Benler, çiller, büyük damarlar, koyu pigmentli alanlar, yara izleri ve cilt anormallikleri üzerinde doktor gözetimi olmadan.
- Cildin yanmasına ve pigmentasyonunun değişmesine neden olabileceğinden dövmelerde veya kalıcı makyajda.
- Cilt tahrişine neden olabileceğinden uzun süreli deodorant kullandığınız bölgelerde.
- Bu cihazı güneş yanığı olan, yakın zamanda bronzlaşmış veya yapay bronzlaşmış cilt üzerinde kullanmayın.

Aşağıdaki ilaçları veya tedavileri alıyorsanız bu cihazı KULLANMAYIN:

- Cildiniz alfa-hidroksi asitler (AHA'lar), beta-hidroksi asitler (BHA'lar), topikal izotretinoin ve azelaik asit ile tedavi ediliyorsa veya yakın zamanda tedavi edildiyse.
- Son altı ay içinde oral veya topikal Accutane veya Roaccutane asit aldıysanız. Bu uygulama cildi yırtılmalara, travmaya ve tahrişe karşı daha duyarlı hale getirir.
- Herhangi bir fotosensitize edici ajan ajan veya ilaç kullanıyorsanız, her zaman ilacın hasta bilgilendirme broşürünü doğrulayın ve ışık alerjisi reaksiyonlarına, foto-toksik reaksiyonlara neden olabileceği belirtiliyorsa veya ilacı aldıktan sonra güneş maruz kalmaktan kaçınmanız gerekiyorsa cihazı kullanmayın.
- Çok miktarda aspirin kullanımı da dahil olmak üzere pıhtılaşmayı önleyici ilaçlar alıyorsanız ve her uygulamadan en az bir hafta önce kesemiyorsanız.
- Herhangi bir rahatsızlık hissederseniz cihazı kullanmayı derhal BIRAKIN ve bir doktora danışın.
- Yangın veya yanık riskini önlemek için ekipman açıkken gözetimsiz bırakmayın.
- Bu ekipman, gözetim altında tutulmadıkları veya ekipmanın kullanımı hakkında bilgilendirilmedikleri sürece, fiziksel, duyusal veya zihinsel yetenekleri sınırlı olan veya deneyim ve bilgi eksikliği olan kişiler tarafından kullanılmak üzere tasarlanmamıştır.
- Bu ekipman çocuklar tarafından kullanılmak üzere tasarlanmamıştır. Çocuklardan uzak tutun. Bu bir oyuncak değildir, şarj kablosu boğulmaya neden olabilir.
- Su ve elektrik tehlikeli bir kombinasyondur! Elektrik çarpması riskini önlemek için:
- bu ekipmanı ıslak ortamlarda kullanmayın (örn. banyoda veya duş ya da yüzme havuzu yakınında);
- cihazın içine su girmesine izin vermeyin.
- Elektrik çarpması riskini veya ekipmanda kalıcı hasarı önlemek için ekipmanı bağlamadan önce ekipmanın üzerinde belirtilen voltajın yerel şebeke voltajına uygun olup olmadığını kontrol edin.
- Ekipmana güç sağlamak için kullanılan duvar prizinin bağlantıları zayıfsa, ekipmanın fişi ısınır. Yangın ve yanık riskini önlemek için ekipmanı düzgün monte edilmiş bir duvar prizine taktığınızdan emin olun.
- HASTANIN, KULLANICI olması hedeflenmiştir.
- Cihaz kullanılmadayken bakım ve onarım yapmayın.
- Cihazı, bağlantı kesme cihazını çalıştırmayı engelleyecek şekilde yerleştirmeyin.
- Cihazın sürekli güvenliğini sağlamak için periyodik olarak önleyici muayene ve bakım yapılmalıdır.
- Ortam sıcaklığı 20°C olduğunda, cihazın kullanımlar arasında minimum depolama sıcaklığından amaçlanan kullanıma hazır hale gelene kadar ısınması için en az 10 dakika gereklidir.

⚠ **DİKKAT**

- Cihaz hasar görmüşse, elektrik çarpmasını önlemek için cihazın iç bileşenlerine DOKUNMAYIN.
- Cihazın içine herhangi bir nesne SOKMAYIN.
- Ürün adaptöründe bir transformatör bulunmaktadır, tehlikeli olabileceğinden güç dönüştürücüyü keserek yerine başka bir fiş TAKMAYIN.
- Işık çıkış penceresinin filtresi hasarlıysa cihazı KULLANMAYIN.
- Kullanım ömrünü uzatmak için cihaz yüzeyini düzenli olarak temizleyin.
- Kazaları önlemek için cihazı kendi başınıza sökmeye, onarmaya veya değiştirmeye ÇALIŞMAYIN.
- Yangın riskinden kaçınmak için bu cihazı yanıcı maddelerin/çözeltilerin/gazların bulunduğu veya oksijenden zengin ortamlarda KULLANMAYIN
- Bu cihazı kullanırken, göz rahatsızlığını önlemek için siz (ve aynı odadaki diğer kişiler) ışık çıkış penceresine doğrudan bakmayın. Cihazı kullanırken DAİMA (ürünle birlikte verilen) koruyucu gözlük kullanın.
- Kullanım sırasında havalandırma deliğini KAPATMAYIN.
- Kabloyu boynun etrafına SARMAYIN.
- Üretici tarafından sağlananlar dışında güç adaptörü KULLANMAYIN.
- Bu cihaz tek kullanıcı için tasarlanmıştır.
- Cihazı güneşlendikten sonra KULLANMAYIN.
- Cildinizin bronzlaşmış mı yoksa yanmış mı olduğundan emin değilseniz, lütfen cilt hassasiyeti testi yapın ve 24 saat bekleyin.
- Lütfen kullandıktan sonra adaptörün fişini çekin.
- Uyarı listesi tüm detayları içermemektedir. Bu cihazı kullanıp kullanamayacağınızdan emin değilseniz, lütfen bir doktora danışın.
- Lambanın hasar görme riskini önlemek için ekipmanı ağır darbelere maruz bırakmayın.
- Ekipmanın hasar görme riskini önlemek için kullanımdan sonra ve elektrik kesintisi durumunda daima fişini çekin.
- Tüy, toz, ışık (güneş ışığı dahil) cihazınızı etkileyebileceğinden lütfen ürününüzü bu tür durumlarda ve ortamlarda kullanmaktan veya saklamaktan kaçının.
- Lütfen ürününüzün evcil hayvanlar ve çocuklar tarafından erişilemeyeceğinden emin olun.

2. Semboller

~	Alternatif akım	⇈	Alternatif akım
⎓	Doğru akım		Doğru akım
▣	SINIF II ekipman		SINIF II ekipman
⚠	Dikkat		Dikkat
⚠	Uyarı		Uyarı

	BF tipi uygulanan parça		Cihaz, kullanım ömrünü tamamladıktan sonra ayrıştırılarak toplanması için yerel yönetmeliklere uygun olarak ilgili kuruluşlara gönderilmelidir.
	Kullanım kılavuzuna başvurun.		Bu cihaz MR ortamında kullanım için test edilmemiştir ve hastalar cihazla birlikte MR ortamlarına maruz kalmamalıdır. MRG tarayıcı odasının dışında tutun.
	Üretici firma		Koruyucu gözlük takın
SN	Seri numarası		Dikkatli kullanılmadığı takdirde kırılabilecek veya hasar görebilecek bir tıbbi cihazı ifade eder.
	Işık kaynaklarından korunması gereken bir tıbbi cihazı ifade eder.		Nemden korunması gereken bir tıbbi cihazı ifade eder.
FC	Federal İletişim Komisyonu		

3. Cihaz Açıklaması

Yoğun Atımlı Işık (IPL) Sistemi, IPL teknolojisine göre çalışan bir epilasyon cihazıdır. Cilt yüzeyinin alt tabakasında çalışır. Cihaz sadece harici güç adaptörü ile çalışır ve IPL emisyon aktivasyonu parmak anahtarı ile yapılır. IPL ışığının amacı tüylerin büyüdüğü kökleri ısıtmaktır. Cihaz, Yoğun Atımlı Işık (IPL) teknolojisine sahiptir.

Cihaz, 18 yaş üstü yetişkinlerin kullanımı için tasarlanmıştır.

3.1. Genel tanıtım
Cihaz Adı: Yoğun Atımlı Işık (IPL) Sistemi
Model: PC-L10001

3.2.Kullanım endikasyonları
Yoğun Atımlı Işık (IPL) Sistemi, istenmeyen vücut tüylerinin giderilmesine yönelik reçetesiz satılan bir cihazdır.

3.3.Cihazın tanıtımı
3.3.1.Cihazın resmi

Ana ünite (resim 1):

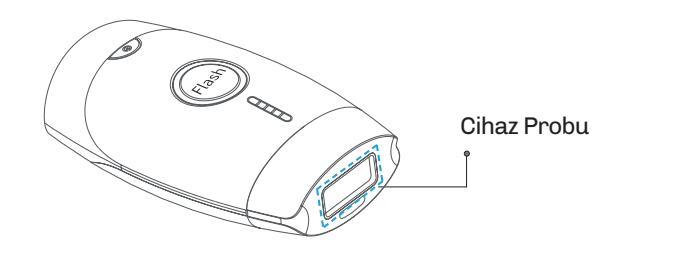

Güç Adaptörü (resim 2):

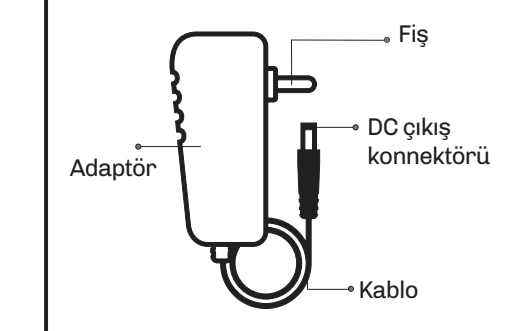

Gözlük (resim 3):



3.3.2.Ana ünitenin konfigürasyonu

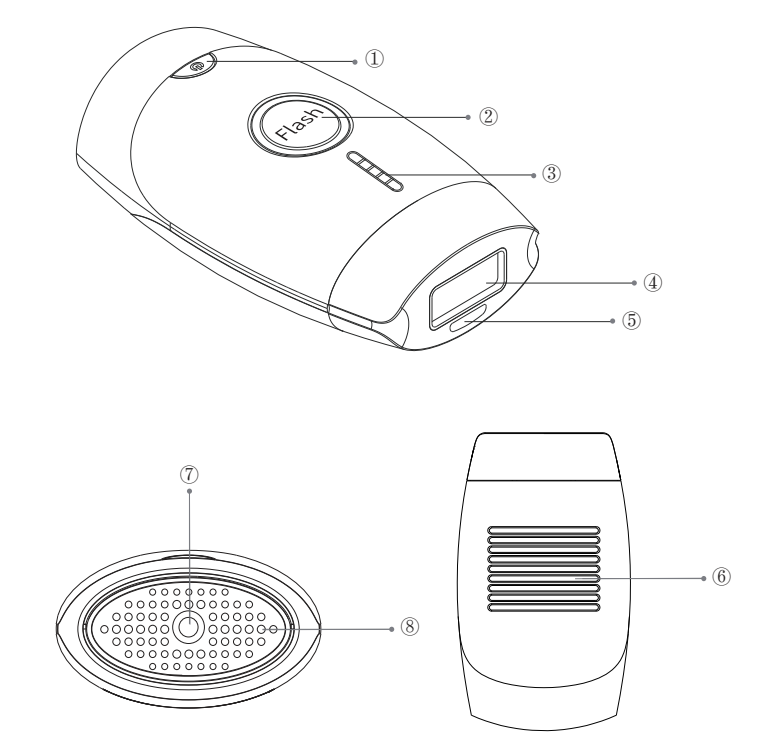

1-Açma/Kapama / Seviye ayar düğmesi
2-Işık Atımı Düğmesi
3-Yoğunluk Seviyesi/Işık Atımına Hazır Işığı
4-Işık Çıkış Penceresi (4cm2)
5-Işık Atımına Hazır Işığı
6-Hava Kanalları (Hava girişi)
7-DC Bağlantı Portu
8-Hava Kanalları (Hava çıkışı)

Işık Atımına Hazır Işığının Durumu	Cihazın durumu	Grafiksel gösterim
Sürekli yanan ışık	"Manuel Işık Atım modunda", Cihaz probu ciltle tam temas halinde değildir.	
Yanıp sönen ışık	1. "Manuel Işık Atım modunda", Cihaz probu cilde tam olarak temas eder ve cihaz ışık atımına hazırdır; ancak henüz Işık Atım Düğmesine basmamışsınızdır. 2. "Otomatik Işık Atım modunda", Cihaz probu cilt ile tam temas halinde değildir.	

4.Cihazın Kullanımı

Bu cihazın doğru çalışmasını sağlamak için lütfen kullanmadan önce talimatları dikkatlice okuyun.

4.1.Cihazın Çalışmasına Giriş
- Hazırlık: Güç adaptörünü ve ana üniteyi aşağıdaki resim 4'teki gibi bağlayın:

Resim 4

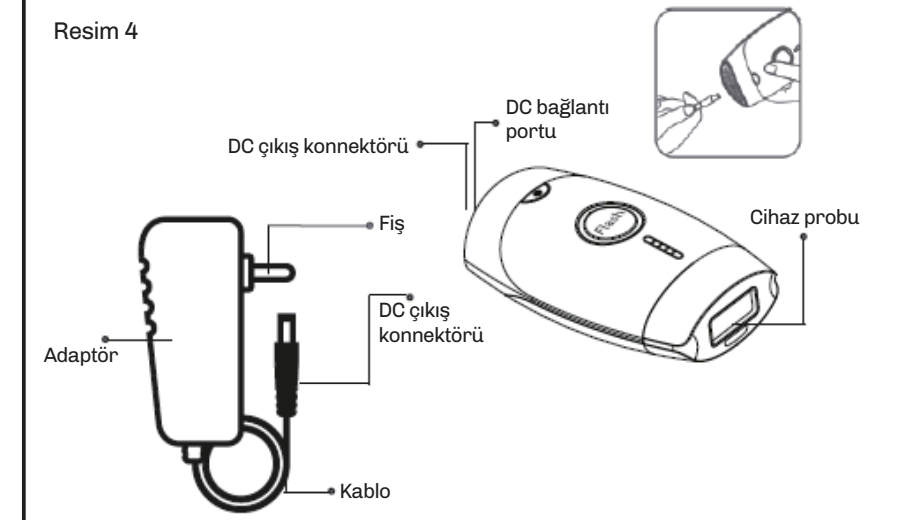

Fişi prize taktıktan sonra cihaz bekleme durumuna geçer ve yoğunluk ışıkları 1 saniye boyunca yanar.

- Cihazın açılması: Cihaz bekleme modundayken, "Açma/Kapama/Seviye ayar düğmesi"ni yaklaşık 2 saniye basılı tutun. Cihaz birinci yoğunluk seviyesinde açılacaktır. Aynı zamanda fan da çalışmaya başlar. (Resim 5)

Resim 5

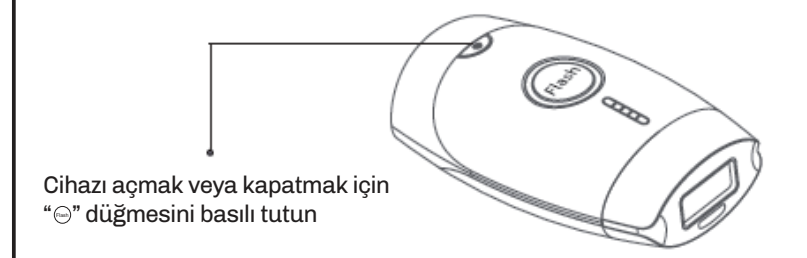

Cihazı açmak veya kapatmak için "○" düğmesini basılı tutun

- Cihazın kapatılması: "Açma/Kapama/Seviye ayar düğmesini" yaklaşık 2 saniye basılı tutun. Yoğunluk Seviye Işıkları ve Işık Atımına Hazır Işığı sönecek ve cihaz bekleme durumuna geçecektir.
- Yoğunluk Seviyesi Ayarı: Cihaz açıkken, uygulama yoğunluğu seviyesini toplam 5 seviyeden oluşan bir döngü içinde ayarlamak için "Açma/Kapama / Seviye ayar düğmesine" basın. İlk kez kullananlar, ilk seansa en düşük yoğunluk seviyesinde başlamalıdır. Yoğunluk seviyesini kademeli olarak artırabilirsiniz. (Resim 6)

Resim 6

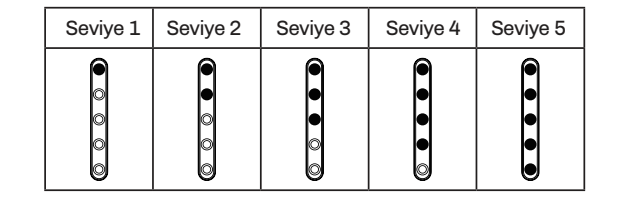

- Manuel Işık Atım modu:
(1)Cihaz açıkken, cihaz otomatik olarak "Manuel Işık Atım moduna" girer.
(2)Cihaz probunu uygulanacak bölgeye yerleştirin ve bastırın (Resim 7).

Resim 7



(3)Işık Atımına Hazır Işığı yanıp sönerek yandığında, Işık Atım Düğmesine basarak ışık atımını tetikleyin. (Resim 8)

Resim 8



Işık atımı için "○" düğmesine basın.

Notlar: 1). "Manuel Işık Atım modunda", Cihaz probu ciltle tam temas halinde değilse, Işık Atımına Hazır Işığı yanar ve Işık Atım Düğmesine "○" basıldığında cihaz ışık atımı yapmaz.
2). "Manuel Işık Atım modunda", Cihaz probu cilde tam olarak temas ediyorsa ancak ışık atımını tetiklemek için Işık Atım Düğmesine basılmazsa ○ Işık Atımına Hazır Işığı yanıp sönerek yanacaktır.
3). Işık Çıkış Penceresi cilde yakınsa ve hareket etmiyorsa ve 8 saniye boyunca sürekli olarak ışık atımı yapılırsa, Işık Atımına Hazır Işığı sürekli olarak yanacak ve cihaz ışık atımını durduracaktır.
4). Küçük alan epilasyonu için "Manuel Işık Atım modu" önerilir.
- Otomatik Işık Atım Modu: Cihaz "Manuel Işık Atım modundayken", Işık Atım Düğmesini yaklaşık 2 saniye boyunca basılı tutun. ○ Cihaz "Otomatik Işık Atım moduna" geçer ve Işık Atımına Hazır Işığı sürekli olarak yanıp söner. Cihaz probunu uygulanacak bölgeye bastırın, cihaz Işık Atım Düğmesine basmadan otomatik olarak ışık atımı yapacaktır.

Otomatik Işık Atım modu altındaki parametre

Seviye	Maruz kalma süresi	Atım miktarı (sayısı)	Her atımın enerji yoğunluğu (J/cm2)	Her ışık atımının süresi	Işık atımları arasındaki süre
1	8s	6x2	1.4±20%	4-12ms	0.5s-6s
2	8s	5x2	1.95±20%	4-12ms	
3	8s	4x1	2.55±20%	4-12ms	
4	8s	3x1	3.2±20%	4-12ms	
5	8s	3x1	3.73±20%	4-12ms	

Notlar:
4). "Otomatik Işık Atım modunda", Cihaz probu cilde tam temas etmiyorsa, Işık Atımına Hazır Işığı sürekli olarak yanıp söner ve cihaz ışık atımı yapmaz.
2). Işık Çıkış Penceresi cilde yakınsa ve 8 saniye boyunca sürekli olarak ışık atımı yapılırsa, Işık Atımına Hazır Işığı sürekli olarak yanıp sönecek ve cihaz ışık atımını durduracaktır.
3). "Otomatik Işık Atım modu" geniş alan epilasyonu için önerilir.
4) TÜM ALANDA uygulama yapıldığından emin olun, ancak atımları üst üste BİNDİRMEYİN.

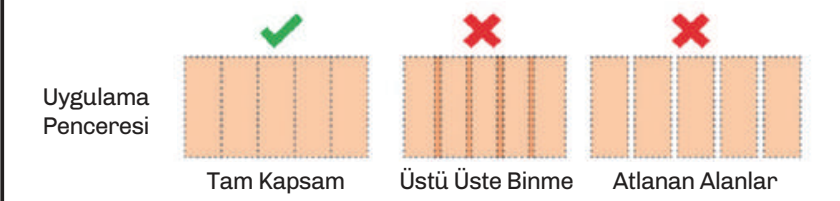

- Mod anahtarı: Cihaz çalışırken, cihazı ciltten uzaklaştırın, Işık Atım Düğmesine yaklaşık 2 saniye basılı tutun; Işık Atımına Hazır Işığı yanıp sönüyorsa, cihaz "Otomatik Işık Atım moduna" geçmiştir. Işık Atım Düğmesine yaklaşık 2 saniye basılı tutun; Işık Atımına Hazır Işığı yanıyorsa, cihaz "Manuel Işık Atım modunda" geçmiştir.

4.2.Cilt Yama Testi
- İlk kez kullanacaklar için, aşağıdaki cilt yama testi ile cihazı kolunuzda reaksiyonlar açısından test etmeniz önerilir:
a.Cihazı açın, yoğunluk seviyesi 1'i seçin, Cihaz probunu cilt üzerine bastırın ve bir ışık atımı uygulayın.
b.24 saat bekleyin ve cildinizde rahatsızlık veya ağrı gibi herhangi bir reaksiyon olup olmadığını kontrol edin.
c.Test bölgesindeki cilt normalse (rahatsızlık veya ağrı yoksa) kullanmaya devam edebilirsiniz, anormalse lütfen kullanmayı bırakın.
d.Yoğunluğu bir seviye artırın ve cihazı bir sonraki alana kaydırın (aynı alanda birden fazla kez ışık atımı yapmayın). Her bir yoğunluk seviyesini yukarıdaki a) ila c) adımlarına göre test edin. Yoğunluk seviyesini artırmayı durdurun ve cihaz herhangi bir rahatsızlığa (veya ağrıya) neden olduğunda testi sonlandırın. Örnek: Yoğunluğu 2. seviyeye yükseltebilir ve yalnızca cihaz 1. seviyede herhangi bir rahatsızlığa (veya ağrıya) neden olmadığında yukarıdaki a) ila c) adımlarına göre test edebilirsiniz.
- Cildinizi test ettikten sonra, cildinizde bir reaksiyona neden olmayan yoğunluk seviyelerini seçin.
- Cildinizin uygulamaya karşı olumsuz bir reaksiyon gösterip göstermediğini doğrulamak için yama testini uyguladıktan sonra her seferinde 24 saat bekleyin. Gözle görülür bir reaksiyon yoksa cihazı kullanabilirsiniz.

4.3.Kullanım Önerileri
- Cihazı kullanmadan önce tüylerinizi yolma, ağda gibi uzun süre etkili bir temizleme yöntemi kullanarak aldıysanız, cihazı kullanmak için tüylerin tekrar çıkmaya başlamasını bekleyin.
- **Uygulama alanları**
Vücut bölgeleri için uygundur: koltuk altı ve çene çizgisinin altındaki yüz tüyleri gibi küçük alanlar ve bacaklar gibi geniş alanlar.
- **Uygulama süresi**
Tüylerin büyüme döngüsüne göre, IPL Epilasyon Cihazının ilk 3-4 kez iki haftada bir kullanılması ve tüylerin durumuna göre kullanımın kademeli olarak azaltılması önerilir.
- **Cilt tonu/tüy rengi referans tablosu**
Lütfen cihazı kullanmaya başlamadan önce cilt tonunuzun ve tüy renginizin kullanıma uygun olup olmadığını belirlemek için aşağıdaki tabloya bakın ("√" cihazın sizin için uygun olduğu anlamına gelir; "X" cihazın sizin için uygun olmadığı anlamına gelir).

Daha koyu cilt tonları ışığı daha kolay emerek ciltte tahrişe neden olur. Bu nedenle, daha koyu cilt tonlarına sahip kişilerin daha düşük ışık atımı yoğunluklu bir ışık kullanmaları önerilir. Kahverengi cilt tonu için lütfen en düşük hız modundan başlayın ve hız ayarını ağrı hissinize göre ayarlayın.

Cilt Tonu:

Ürün Tip I'den Tip IV'e kadar olan cilt tonları için uygundur. Lütfen cilt tonunuzu belirleyin ve ürünün size uygun olup olmadığını görmek için aşağıdaki tabloyu kontrol edin.

Cilt Tonu Tablosu:

Cilt tipi/rengi	Görünüm	Güvenlik sınıfı
Tip I Soluk beyaz ten	✓	Uygulanabilir
Tip II Beyaz ten	✓	Uygulanabilir
Tip III Krem beyazı ten	✓	Uygulanabilir
Tip IV Orta kahverengi ten	✓	Uygulanabilir
Tip V Koyu kahverengi ten	✗	Geçerli değil
Tip VI Derin pigmentli koyu kahverengi ila en koyu kahverengi, siyah ten	✗	Geçerli değil

TÜY RENGİ:
IPL sistemi, doğal siyah veya kahverengi tüylerde kullanım için uygundur. Beyaz, gri, sarı veya kızıl tüylerde o kadar etkili olmayabilir.

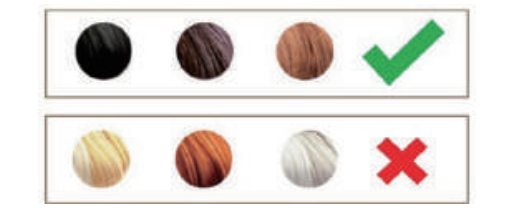

4.4.Kullanım Adımları
- Cihazı kullanmaya başlamadan önce, cilt yüzeyindeki tüm tüyleri tıraş etmek için bir tıraş bıçağı veya saç kesme makinesi kullanın (tüyleri yolmayın veya kimyasal epilasyon ürünleri kullanmayın) (şekil 9), cildi tamamen kurulayın ve yağlı maddeleri (vücut kokusu, losyon, parfüm, güneş kremi ve diğer kozmetikler gibi) temizleyin.



Şekil 9

- Güç adaptörünü ana üniteye bağlayın ve ardından fişi bir elektrik prizine takın.
- Cihazı açmak için "Açma/Kapama/Seviye ayar düğmesini" basılı tutun.
- Cilt tonunuza ve tüy renginize uygun ışık atımı yoğunluğunu seçin (ilk kez kullanacaklar için önerilen en düşük ışık yoğunluğunu kullanın ve kademeli olarak ayarlayın).
- Işığa bakmaktan kaçınmak için koruyucu gözlük takın (Şekil 10).



Şekil 10

- Cihaz probunun ciltle tam olarak temas ettiğinden emin olarak Cihaz probunu cilde bastırın (Şekil 11). Birkaç saniye bekleyin, Işık Atımına Hazır Işığı yanıp sönmeye başladığında, ışık atımı yapmak için Işık Atım Düğmesine basın. Hafif bir yanma hissedeceksiniz (ışık atımı enerjisi absorbe edilir). Yanma hissini azaltmak istiyorsanız, uygulama seviyesini ayarlayın.



Şekil 11

- Kullandıktan sonra cihazı kapatın, güç adaptörünün fişini çekin ve cihazı temizleyin.

Not:
1.Cihazın ana ünitesinde, cihazın çalışması sırasında ana ünitenin iç parçalarını soğutmak için kullanılan bir fan bulunur. Cihaz çalıştırıldığında, fan cihaz kapanana kadar sürekli rüzgar sesi çıkararak çalışmaya başlar.
2.Güç adaptörünü prizden çıkardıktan 20 dakika sonra cihazı bu kılavuzun 6. bölümüne göre temizleyin.
3.Temizledikten sonra, cihazı ve adaptörü kutusuna geri koyun ve belirtilen saklama koşullarına uygun olarak saklayın.

⚠ **DİKKAT**
1.Cihazı kullandıktan sonra cildinize herhangi bir parfümlü cilt bakım veya kozmetik ürünü UYGULAMAYIN.
2.Cihazı koltuk altlarında kullandıktan hemen sonra deodorant KULLANMAYIN. Deodorant kullanmaya başlamak için ciltteki kızarıklığın tamamen geçmesini bekleyin.
3.Her uygulamayı takiben 24 saat sonra cildinizde herhangi bir kızarıklık belirtisi olmadığından emin olun.
4.Uygulamadan sonraki iki hafta boyunca uygulama yapılan bölgeyi kapalı ve doğrudan güneş ışığından uzak tutun veya uygulama yapılan bölgeye güneş kremi (SPF30+) sürün.

5. Nadir Yan Etkiler

- Yanıklar, anormal kızarıklık ve şişlik
Bu reaksiyonlar çok nadir görülür. Yüksek ışık atımı yoğunluğu kullanmaktan kaynaklanıyor olabilir. Bu istenmeyen reaksiyonlar 3 gün veya daha uzun süre devam ederse, derhal bir doktora başvurun. Bir sonraki uygulamaya yalnızca ciltte herhangi bir sorun yoksa başlayın ve daha düşük bir ışık atımı yoğunluğu kullandığınızdan emin olun.
- Ciltte renk değişikliği
Normal ama çok nadir. Cihazı kullanırken cildinizde renk değişikliği olabilir, bunun nedeni yüksek yoğunluklu ışık atımı kullanmanız olabilir. Renk değişikliği kaybolduğunda, sonraki uygulamalar sırasında ışık atımı yoğunluğunu azaltın. Ciltteki renk değişikliği iki hafta sonra kaybolmazsa, lütfen bir doktora danışın.
- Cilt enfeksiyonları ve iltihapları
Çok nadir. Cihaz mevcut yara ve kesiklerde kullanılırsa (bölgeyi tıraş ederken olabilir) belirtilen yan etkilere neden olabilir.
- Uygulama sırasında ve sonrasında aşırı ağrının olası nedenleri
Cihazı uygulamaya başlamadan önce tıraş edilmemiş bir bölgede kullandınız; ışık atımı yoğunluğu cilt tonunuz ve tüy renginiz için çok yüksektir; cihazı aynı bölgede birden fazla kez kullandınız; cihazı açık bir yarada kullandınız; uyguladığınız bölgede herhangi bir iltihap veya enfeksiyon varsa; cihazı dövme veya güneş yanığı olan bölgelerde kullanıyorsanız.

6. Temizlik ve Bakım

6.1.Temizlik
Her kullanımdan sonra, bu cihazı aşağıdaki ipuçlarını izleyerek temizleyin:

Amacı: Bu cihaz istenmeyen tüyleri almak için tekrar kullanılmak üzere tasarlanmıştır. Kullanım sırasında insan eliyle taşınan organik maddeler ve mikroorganizmalarla kirlenebilen cihaz yüzeyini her kullanımdan hemen sonra temizleyin.
Temizlik Malzemesi: Silmek için %70 izopropil alkol kullanın.
Temizleme Yöntemi: Her kullanım sonrasında cihazı iyice temizlemek için işlemi hemen gerçekleştirin. Işık Çıkış Penceresi, kapak, düğme gibi parçaları (etiketler dahil) elinizde aşırı basınçlı uygulamadan %70 izopropil alkol ile 15 saniye ve Işık Çıkış Penceresini 3 saniye boyunca silin.

Not:
1.Cihazın içine sıvı kaçmadığından emin olun.
2.Temizlik için ASLA aşındırıcı temizlik malzemeleri, tiner veya benzen kullanmayın.
3.Cihazı ASLA suya veya diğer temizlik sıvılarına daldırmayın.
4.Temizlikten sonra cihazın kuruması için 10 dakika bekleyin.

Görsel İnceleme: Temizlikten sonra, doğa ışığı altında cihaz üzerinde gözle görülür kir ve leke kalmamalıdır, eğer hala kir ve/veya leke varsa, herhangi bir kir ve leke kalmayana kadar yukarıda belirtilen temizlik adımlarını tekrarlayın.

Temizlikten sonra korozyon, renk değişikliği, çukurlaşma veya çatlaklar varsa, cihazın çevre dostu ve uygun şekilde bertaraf edilmesi için seçenekler hakkında bilgi alın. Yerel düzenlemeleri dikkate alın.

Yeniden Kullanım Ömrü: 999.999 ışık atımı

6.2.Bakım
- Işık Çıkış Penceresi çok hassastır. Işık Çıkış Penceresini kir ve hasardan korumak çok önemlidir. Pencereye dokunmayın veya basmak için herhangi bir alet kullanmayın. Dikkatli bir şekilde korunmalıdır.
- Bu cihaz su geçirmez değildir. Suya DALDIRMAYIN veya akan suyun altında YIKAMAYIN.
- Cihazı temizlemek için bulaşık teli, aşındırıcı temizleyiciler, kimyasallar veya aşındırıcı sıvılar KULLANMAYIN.

7. Saklama

Cihazı uzun süre sıcak veya nemli bir ortamda BIRAKMAYIN veya SAKLAMAYIN. Bu cihazı aşağıdaki koşullarda saklayın:

Saklama koşulları	Sıcaklık: -20 ~ 55°C Bağıl nem: %5 ~ 95, yoğuşma olmadan Atmosfer Basıncı: 70 kPa ~ 106 kPa

8. Geri Dönüşüm

Kullanım ömrünün sona erdiğinde, bu cihazı evsel atıklarla birlikte atmayın. Lütfen bu cihazı uygun şekilde yerel bir geri dönüşüm noktasına götürün. Uygun bertaraf ve geri dönüşüm uygulamaları çevrenin korunmasına katkıda bulunur.

9. Garanti ve Destek

Sorun	Olası Neden	Çözüm
Gösterge ışığı kapalı	Güç kablosu düzgün bağlanmamıştır.	Güç kaynağının bağlantısını kontrol edin ve kabloyu ayarlayın.
	Sadece "Açma/Kapama /Seviye ayar düğmesine" basın, ancak basılı tutmayın.	Cihazı açmak için "Açma/ Kapama/Seviye ayar düğmesini" yaklaşık 2 saniye basılı tutun.
Cihaz ışık atımı yapmıyor.	Güç kablosu doğru bağlanmamıştır.	Güç kaynağının bağlantısını kontrol edin ve kabloyu ayarlayın.
	Cihaz probu cilde yeterince yakın değil	Işık Atımına Hazır Işığı yanıp sönmeye başlayana kadar Cihaz Probunun cildinizdeki konumunu yeniden ayarlayın.
Kullanım sırasında cihaz bekleme moduna giriyor.	Cihaz, 5 dakika içinde ışık atımı yapılmazsa otomatik olarak kapanıyor.	Cihazı açmak için "Açma/Kapama/Seviye ayar düğmesini" yaklaşık 2 saniye basılı tutun.
Cihaz tuhaf bir koku çıkarıyor.	Işık çıkış penceresi filtresi kirlidir.	Işık çıkış penceresi filtresini %70 izopropil alkol ile dikkatlice silin.
	Tüyler uygulamadan önce uygun şekilde alınmamıştır. Işık atımı tüyleri yakarak tuhaf bir kokuya neden olur.	Cihazı kullanmaya başlamadan önce, uygulamak istediğiniz bölgedeki tüm tüyleri bir tıraş bıçağı veya saç kesme makinesi ile alın.
Cihazı kullanırken canınız yanıyor.	Işık atımı yoğunluğu çok yüksektir.	Işık atımı yoğunluğunu düşürün ve azaltın.
	Işık çıkış penceresinin filtresi hasar görmüştür.	Lütfen cihazı kullanmayı bırakın ve yardım için bölge bayinize başvurun.
	Cihazı uygulanabilir olmayan bir alanda kullanıyorsunuz.	Lütfen kullanım kılavuzunu, uyarıları ve belirtilen kullanım yasaklarını okuyun.
Cihazı kullandıktan sonra, uyguladığı bölge kızarıklık belirtileri gösteriyor.	Hafif kızarıklık epilasyona karşı normal ve zararsız bir reaksiyondur.	Normal bir tepki olduğu için herhangi bir işlem yapmaya gerek yoktur.
Uygulama sonuçları tatmin edici değil.	Kullanılan ışık atımı yoğunluğu çok düşüktür.	Bir dahaki sefere kullanırken ışık atımı yoğunluğunu ayarlayın.
	Frekansı önerilenden daha düşüktür.	Cildin pürüzsüz ve tüysüz kalması için cihazın iki haftada bir kullanılması önerilir. Uygulama aralıkları her kişinin tüy büyüme döngüsüne bağlıdır. Cihazı iki haftada bir defadan fazla kullanmayın. Aşırı kullanım istenmeyen cilt reaksiyonları riskini artırabilir.
Uygulama sonuçları tatmin edici değil.	Cilt tonunuz ve tüy renginiz bu cihazın kullanımı için uygun değildir.	Vücut tüyleriniz sarı, kızıl, gri, beyaz veya cilt tonunuz çok koyu ise bu cihazı kullanmayın.
Diğer sorunlar.		Bölge bayinizle iletişime geçin.

Not: Yukarıdaki çözümleri uygulamanıza rağmen cihaz hala düzgün çalışmıyorsa, lütfen cihazı kullanmayı bırakın ve bölge bayinizle iletişime geçin.

10. Paketleme Listesi

Ana ünite	1 adet	Güç adaptörü	1 adet
Talimat kitabı	1 adet	Güvenlik gözlüğü	1 adet
Gözlük temizleme bezi	1 adet	Saklama çantası	1 adet

11. Teknik Özellik Parametreleri

Cihaz Adı	Yoğun Atımlı Işık (IPL) Sistemi
Model	PC-L10001
Boyutlar	139,5x83,3x48,3mm
Risk grubu	Muaf Grup
Işınlama alanı	Işık çıkışı: 4,0cm2
Adaptör Girişi	100-240 Va.c. 50/60Hz, 1,5A
IPL ana parça girişi	24 Vd.c, 2,0 A
Dalga boyu	510~1200nm
Maks. Akıcılık	4,5J/cm2
Atım süresi	4 ~ 12ms
Çıkış enerjisi	5,6J-18J
Hizmet ömrü	999.999 ışık atımı
Ağırlık	254,5g
Çalışma ortamı	Sıcaklık: 5 ~ 30°C Bağıl nem: %20 ~ 90, yoğuşma olmadan Atmosfer Basıncı: 70 kPa ~ 106 kPa
Depolama ve taşıma ortamı	Sıcaklık: -20 ~ 55°C Bağıl nem: %5 ~ 95, yoğuşma olmadan Atmosfer Basıncı: 70 kPa ~ 106 kPa
Uygulanan parça	Tip BF
Sterilizasyon gereksinimi yok	
AP / APG ekipmanı kategorisinde değil	
Çalışma modu: sürekli	

Adaptör Teknik özellikler:

Ürün	Parametreler
Adaptör modeli	AK36WG-2400150DP
Giriş Gerilimi	100Vac~240Vac
Giriş Frekansı	50Hz/60Hz
Güç adaptörünün kullanım ömrü	10 yıl
Çıkış voltaj aralığı	22,8 ~ 25,2Vdc
Çıkış akım aralığı	0 ~ 2A
Çıkış gücü	<36W
Aşırı gerilim çıkışı	çıkış geriliminin<%170'i
akım sınırlayıcı koruma	4,5-7,5A

12. Sıkça Sorulan Sorular

S: Cihaz kullanım sırasında otomatik olarak kapanıyor.
C: Cihazın iç sıcaklığı çok yüksek olduğunda cihaz otomatik olarak kapanır, lütfen 10 dakika sonra cihazı yeniden başlatın.

S: Her kullanımdan önce tüyleri tıraş etmem gerekir mi?
C: Hayır. Ancak 5 mm'den uzun olduğunda tüyleri tıraş etmeniz tavsiye edilir.

S: Birkaç kez uyguladıktan sonra tüylerim neden hala uzuyor? Neden uygulamadan hemen sonra dökülmüyor?
C: Yoğun Atımlı Işık (IPL) Sistemi, kıl köküne çok hafif ışık darbeleri uygulayan ev tipi bir IPL epilasyon cihazıdır. Kademeli olarak adım adım çalışır, öncelikle tüy dinlenme aşamasına geçer - sahip olduğunuz tüyler dökülür ve yavaş yavaş vücudunuz o bölgede daha az tüy çıkarır ve son olarak tüylerin tekrar uzaması durur; bu zaman alır.
Kalıcı bir tüy temizleyicidir. Cihazı bir süre kullanmanız tüylerin kalıcı olarak giderilmesi değildir. Sadece tüy büyümesini baskılayabilir ve başlangıçta tüyün uzama hızını yavaşlatabilir. Tüy sürekli hareket halinde uyku durumuna girer. Böylece kalıcı epilasyon etkisi elde edilir.

S: Neden diğerleriyle aynı etkiyi elde edemedim ya da hiç etki elde edemedim?
C: İnsanların farklı fiziksel özellikleri vardır ve tüy kalınlığı ile işleme giren kısımların farklılığı etki döngüsünü etkileyebilir. Kullanım döngüsü ortalama bir değerdir ve spesifik süresi biraz farklı olabilir.

S: Hangi seviye uygundur?
C: Uygun seviyelerin birleşik bir standardı yoktur, hepsi cilt toleransınıza bağlıdır, cilt rengi ne kadar koyu olursa, seviye o kadar düşük kullanılmalıdır. Ve uygun seviyeyi seçmeye en düşük seviyeden başlayın. Seviye ne kadar yüksek olursa, uygulama etkisi o kadar belirgin ve uygulama süresi o kadar kısa olur. Aksine, düşük bir seviye kullanırsanız, uygulama süresi de buna bağlı olarak uzayacaktır. Her epilasyondan önce uygulanan cilt kısmında lokal cilt testleri yapılması ve ardından kiriçi gün cilt rahatsızlığı oluşmadığından emin olduktan sonra geniş cilt alanlarında uygulamaya başlanması önerilir.

S: Can yakar mı?
C: Epilasyon sırasında, ışık dalgaları tüy melaninleriyle karşılaştığında ısı üretecek ve hafif bir acıya neden olacaktır. Farklı bireylerin farklı cilt hassasiyeti ve ağrı toleransı nedeniyle, gerçek hisler farklıdır. Gerçek durumunuza göre seviyeyi en düşükten yavaşça hızlandırmanız önerilir.

S: Nasıl tıraş olunur? Ne tür tüyler tıraş edilmelidir?
C: Genel olarak, kullanmadan önce koltuk altı, bikini bölgesi ve bacaklardaki tüyleri tıraş etmelisiniz. Bu yöntem tıraş olmayı kolaylaştırır:
1.Tıraş bölgesini kayganlaştırmak için tıraş kremi veya yumuşak duş jeli kullanın.
2.Ya da tıraş bölgesine birkaç dakika sıcak havlu uygulayın ve havluyu kaldırdıktan hemen sonra tüyleri nazikçe tıraş edin; bu tıraşı kolaylaştıracaktır.

S: Kullanımdan sonra neden yanık tüy kokusu oluyor?
C: Bunun nedeni tüyün tamamen tıraş edilmemiş olmasıdır. Işık dalgaları kullanılırken melaninle karşılaştığında ısı üretecek ve bu da yanık tüy kokusuna neden olacaktır. Ve bu normaldir.

S: Tüylerimi hızlıca temizlemek istiyorum. Cihazı her gün kullanabilir miyim?
C: Cihazın her gün kullanılması tavsiye edilmez. Tüyün bir büyüme döngüsü vardır; normal döngüye göre kullanabilirsiniz: İlk 3 ~ 4 kez boyunca her iki haftada bir kullanın ve tüy büyümesi yavaşladıktan sonra kullanım sayısını kademeli olarak azaltın.

13. Elektro Manyetik Uyumluluk (EMC) ile İlgili Önemli Bilgiler

⚠ Uyarı: Bu cihazın yakınında cep telefonu veya mikrodalga fırın, yüksek frekanslı cerrahi ekipman, manyetik rezonans görüntüleme veya diğer radyo dalgası yayan ekipmanların kullanılması arızaya neden olabilir veya önemli ölçüde performans kaybına yol açabilir.

⚠ Uyarı: Bu ekipmanın diğer ekipmanlarla bitişik veya üst üste kullanılmasından kaçınılmalıdır çünkü bu durum ekipmanın yanlış çalışmasına neden olabilir. Böyle bir kullanım gerekliyse, bu ekipman ve diğer ekipman normal çalıştıklarını doğrulamak için gözlemlenmelidir.

⚠ Uyarı: Bu ekipmanın üreticisi tarafından belirtilen veya sağlananlar dışında adaptör kullanılması, elektromanyetik emisyonların artmasına veya bu ekipmanın elektromanyetik bağışıklığının azalmasına ve hatalı çalışmaya neden olabilir.

⚠ Uyarı: Taşınabilir RF iletişim ekipmanı (anten kabloları ve harici antenler gibi çevre birimleri dahil), üretici tarafından belirtilen kablolar dahil olmak üzere Yoğun Atımlı Işık (IPL) Sisteminin herhangi bir parçasına 30 cm'den (12 inç) daha yakın kullanılmamalıdır. Aksi takdirde, bu ekipmanın performansında bozulma meydana gelebilir.

---

pierre cardin
PARIS

IPL LAZER EPİLASYON

PC-L10001

pierre cardin
PARIS

CE RoHS

İthalatçı Firma Bilgileri:
Teknokta İç Dış Tic. Ltd. Şti.
Adres: Küçükbakkalköy Mh. Kayışdağı Cd. Ayşe Hatun Çeşme Sk. No:9 Kat:-1,0,1,2 PK: 34775 Ataşehir / İstanbul
Telefon: +90 216 600 20 00 | Fax: +90 216 576 38 78

1. Safety Instructions

Before using the Intense Pulsed Light (IPL) System for the first time, please read the user manual carefully.

⚠ **Warning**

- This device is not a toy, keep out of reach of children.
- Please verify the device before you start using it. DO NOT use if there is any damage.
- Keep the device and power adapter dry.
- Make sure the device operating voltage complies with the rated voltage of the power source.
- Make sure you always wear the goggles during you operate the device.

⚠ **Caution**

- The Intense Pulsed Light (IPL) System is an electrical device. As such, it should be used with special attention to safety. Please read all warnings and cautions before use, and strictly follow them when using the device.

Contraindications:

- The following persons should not use this device:
- Pregnant women or while nursing, or during menstruation; children.
- Your skin is sensitive to light and is prone to develop a rash or allergic reaction.
- You have skin type V and VI(You rarely to never sunburn, very dark tanning)
- In this case you run a high risk of developing skin reactions, such as hyperpigmentation and hypopigmentation, strong redness or burns.
- Persons with a history of skin diseases, Or those are currently being treated for skin related diseases.
- Persons with precancerous lesions or multiple atypical birthmarks (moles) on the areas you want to use the device.
- If the area you want to treat has infections, burns, eczema, hair follicle inflammation,scratches,open wounds, herpes simplex, lacerations or hematomas.
- Persons with a history of collagen disorder, keloid scar formation or Difficulty in healing wounds.
- Persons with a history of vascular diseases, such as varicose veins, etc.
- Persons with diabetes, lupus erythematosus, porphyria, congestive heart disease, and bleeding disorders.
- Persons who have a history of immunosuppressive disease (including HIV infection and AIDS).
- If you are receiving or have received in the last couple of months radiotherapy or chemotherapy.

⚠ **Warning**

- DO NOT use this device on the following areas:
- On areas with hyperpigmentation or hypopigmentation, intense redness, or burns
- On areas where you had surgery.
- Around the eyes and eyebrows to avoid eye injury.
- On the nipples, areolas, labia minora, vagina, anus, inside the nostril and ears.
- Mencannot use this device on the scrotum and face.
- Near silicone implants, pacemakers, subcutaneous injection port (such as insulindispensers), body piercings. Any artificial surface should be avoided.
- On moles, freckles, large veins, darker pigmented areas, scars, and skin abnormalities without doctor supervision.
- On tattoos or permanent makeup, as it can cause burns to the skin and change itspigmentation.
- On areas where you use long-lasting deodorants, as it may cause skin irritation.
- Do not use this device on skin with sunburns, recently tanned or false tanned.
DO NOT use this device if you take the following medications or treatments:
- Your skin is being treated or has recently been treated with alpha-hydroxy acids (AHAs), beta -hydroxide acids (BHAs), topical isotretinoin and azelaic acid.
- If you have taken oral or topical Acutane or Roaccutane acid in the past six months. This treatment makes skin more susceptible to lacerations, trauma, and irritation.
- If you are taking any kind of photosensitizing agent or medication, always verify the patient information leaflet of the medicine, and do not use the device if it is specified that it can cause light allergy reactions, photo -toxic reactions, or if you should avoid sun exposure while taking the medicine.
- If you are taking anticoagulant medicines, including the use of large quantities of aspirin and cannot stop at least one week before each treatment.
- Immediately **STOP** using the device and consult a doctor if you feel any discomfort.
- Do not leave the equipment unattended when it is switched on to avoid the risk of fire or burns.
- This equipment is not intended for use by persons with reduced physical, sensory or mental capabilities, or lack of experience and knowledge, unless they have been given supervision or instruction concerning use of the equipment to avoid the risk of fire or burns.
- This equipment is not intended for use by children. Keep it away from children.
- This is not a toy, the charging cord could lead to strangulation.
- Water and electricity are a dangerous combination! To avoid risk of electrocution.
-do not use this equipment in wet surroundings (e.g. in the bathroom or near a shower or swimming pool);
-do not let water run into the appliance.
- Check if the voltage indicated on the equipment corresponds to the local mains voltage before you connect the equipment to avoid risk of electrocution or permanent damage to the equipment.
If the wall socket used to power the equipment has poor connections, the plug of the equipment becomes hot. Make sure you plug the equipment into a properlyin stalled wall socket to avoid the risk of fire and burns.
- The PATIENT is an intended OPERATOR.
- Do not service and maintain while the device is in use.
- Do not locate the device so that it is difficult to operate the disconnection device.
- Preventive inspection, maintenance shall be performed Periodically to ensure the continued Safety of the device.
- At least 10 minutes is required for the device to warm from the minimum storage temperature between uses until the device is ready for its intended use when the ambient temperature is 20°C.
- At least 10 minutes is required for the device to cool from the maximum storage temperature between uses until the device is ready for its intended use when the ambient temperature is 20°C.

⚠ **Caution**

DO NOT touch the internal parts to avoid electric shock, if the device is damaged.
DO NOT insert any objects into the device.
The adapter contains a transformer, **DO NOT** cut the power converter to replace it with another plug as it is dangerous.
DO NOT use the device if the filter of the light exit window is damaged.
Regularly clean the device surface to extend its lifetime.
DO NOT attempt to disassemble, repair or modify the device by yourself to avoid accidents.
DO NOT use this Device In an environment with flammable materials/ solutions/ gases or Or an oxygen-rich environment to avoid fire risk.
When using this device, ensure you (and other people in the same room) do not look directly into the light exit window to avoid eye discomfort. **ALWAYS** use protective goggles (included) when using the device.
DO NOT cover the vent during use.
DO NOT wrap the cable around neck.
DO NOT use power adapter other than provided by the manufacturer.
This device is for single patient reuse.
DO NOT use the device after Sunbathing.
Please do a cutaneous sensitivity test and wait for 24 hours, if you are not surewhether your skin has been tanned or burned.
Please unplug the adapter after Using.
The warning list is not exhaustive. If you are not sure whether you can or cannot use this device, please consult a doctor.
Do not subject the equipment to heavy shocks to avoid risk of damage to the lamp.
Always unplug the appliance after use and in case of a power failure to avoid risk of damage to the equipment.
Lint, dust, light (including sunlight) can effect your device, please avoid use or Storage of your product in such situation.
Please ensure your product can not be reached by pets, children.

2. Symbols

~	Alternating current	⇈	This way up
⎓	Direct current		Date of manufacture
▣	CLASS II equipment		Temperature limit
⚠	Caution		Humidity limitation
⚠	Warning		Atmospheric pressure limitation

	Type BF applied part		The device should be sent to the s pecial agencies according to local regulations for separate collection after its useful life
	Refer to instruction manual		for use in an MR environment and should not be used exposed to MR environments while patients are wearing the device. Keep it outside the MRI scanner room.
	Manufacturer		Wear eye protection
SN	Serial number		Indicates a medical device that can be broken or damaged if not handled carefully
	Indicates a medical device that needs protection from light sources		Indicates a medical device that needs to be protected from moisture
FC	Federal Communications Commission		

3. Device Description

Intense Pulsed Light (IPL) System is a device for hair removal based on Intense Pulsed Light (IPL). It works below the skin's surface. The device is only powered by the external power adapter and its IPL emission activation is by finger switch, the purpose of the IPL light is to heat the root where the hair grows. The device incorporates Intense Pulse Light (IPL) technology.

The device is intended to be used for adults aged over 18.

3.1. General introduction

Device Name: Intense Pulsed Light (IPL) System
Model: PC-L10001

3.2. Indications for use

The Intense Pulsed Light (IPL) System is an over-the-counter device intended for the removal of unwanted body hair.

3.3. Introduction of device

3.3.1. Device picture

Main unit (picture 1):

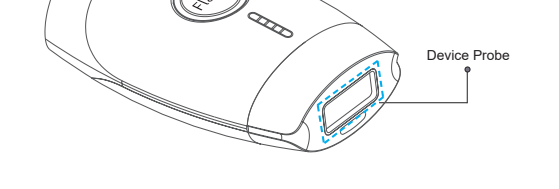

Power Adaptor (picture 2):



Goggles (picture 3):



3.3.2. Configuration of Main unit

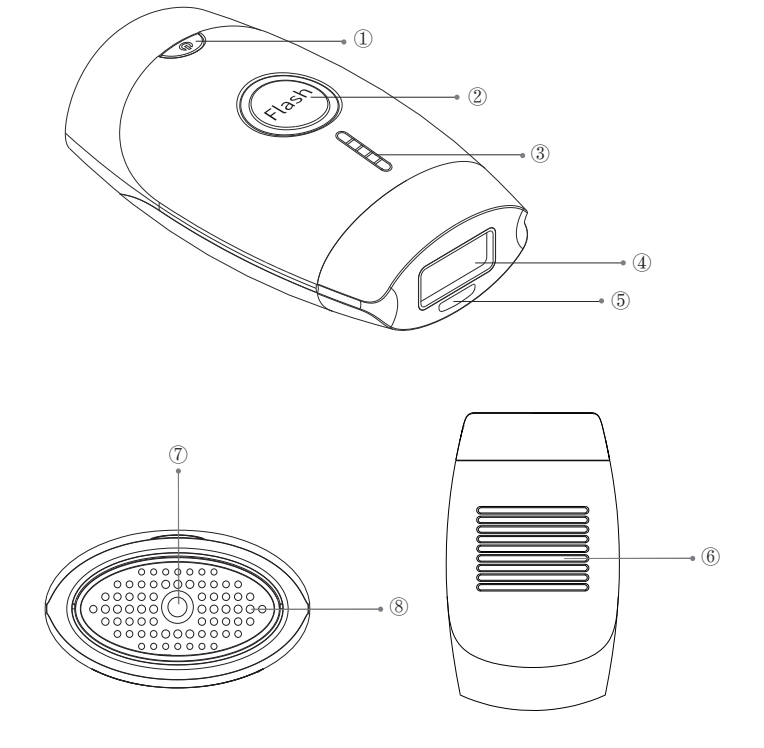

① On/Off / Level adjustment button
② Flash Button
③ Intensity Level/Flash Ready Light
④ Light Exit Window (4cm²)
⑤ Flash Ready Light
⑥ Air Vents (Air inlet)
⑦ DC Plug-in Port
⑧ Air Vents (Air outlet)

Status of Flash Ready Light	When	Graphical representation
Light on	In"Manual Emit Flash mode", the Device probe is not in full contact with the skin.	
Light with blinking	1.In "Manual Emit Flash mode", the Device probe fully contact the skin and device is ready to trigger a flash, but you haven't pressed the Flash Button ○ yet. 2. In "Auto Emit Flash mode", the Device probe isnot in full contact with the skin.	

4. How to use

To ensure the correct operation of this device, please read the instructions carefully before use.

4.1. Device Operation Introduction

- **Preparation:** Connect power adaptor and main unit like following picture 4:

Picture 4:

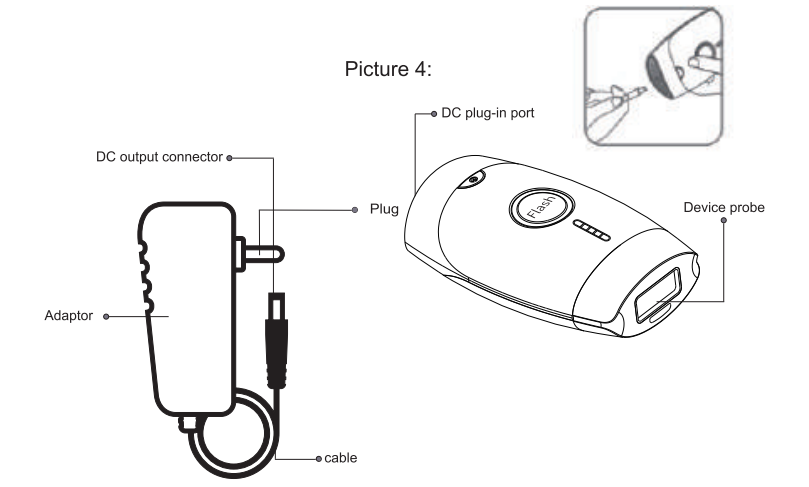

After inserting the plug into a power socket, the device gets in standby state and the intensity lights light up for 1 second.

- **Power on**: With the device in standby, press and hold the "On/Off/Level adjustment button"for about 2 seconds, the device will be powered on at the first intensity level, At the same time, the fan begins working. (Picture 5)

Picture 5

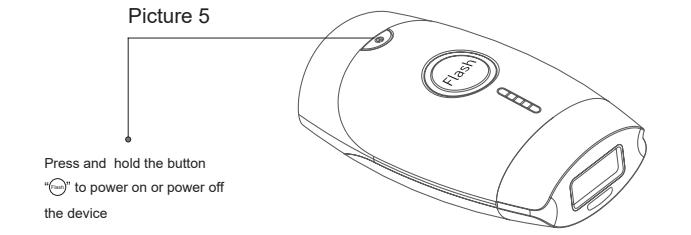

Press and hold the button ○ to power on or power off the device

Power OFF: Press and hold the "On/Off/Level adjustment button" for about 2 seconds, the Intensity Level Lights and the Flash Ready Light will go out, the device gets in standby state.
Intensity Level Adjustment: With the device Powered on, press the "On/Off/ Level adjustment button" ○ to adjust the treatment intensity level in a cycle-a total of 5 levels.First-time users should start the first session at the lowest intensity level. You can gradually increase the intensity level. (Picture 6)

Picture 6

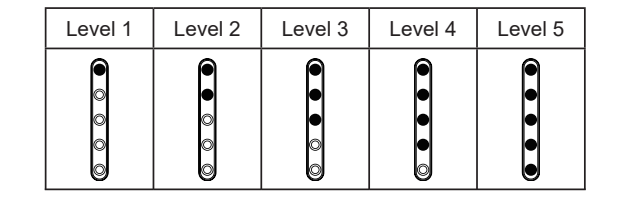

- **Manual Emit Flash mode:**
(1)With the device Powered on, the device automatically enters "Manual Emit Flash mode".
(2)Put the Device probe against the area to be treated and press (Picture 7)

Picture 7



(3)When Flash Ready Light is light with blinking, press the Flash Button ○ to trigger a flash. (Picture 8)

Picture 8



Press the button "○"to trigger a flash

Notes: 1). In "Manual Emit Flash mode", if the Device probe is not in full contact with the skin, the Flash Ready Light will light on and the device does not emit the fash when pressing the Flash Button" ○ "
2). In "Manual Emit Flash mode", if the Device probe fully contact with the skin but not press the Flash Button " ○ " to trigger a flash, the Flash Ready Light will ligh with blinking.
3). If the Light Exit Window is close to the skin and does not move, and the flash is continuously exposed for 8 second, Flash Ready Light will be light without blinking and device stop emitting flash.
4)."Manual Emit Flash mode" is recommended for small area hair removal.

- **Auto Emit Flash mode**: With the device in "Manual Emit Flash mode", press and hold the Flash Button " ○ "for about 2 seconds, the device is into "Auto Emit Flash mode" and Flash Ready Light lights with blinking, press the Device probe against the area to be treated, the device will emit the flash automatically without pressing the Flash Button.

The parameter under Auto Emit Flash mode

Level	Exposure time	Quantity of pulses (times)	Energy density of each pulse (J/cm²)	Pulse duration of each flash	Interval time between flashes
1	8s	6x2	1.4±20%	4-12ms	0.5s-6s
2	8s	5x2	1.95±20%	4-12ms	
3	8s	4x1	2.55±20%	4-12ms	
4	8s	3x1	3.2±20%	4-12ms	
5	8s	3x1	3.73±20%	4-12ms	

Notes:
1). In "Auto Emit Flash mode", if the Device probe is not in full contact with the skin, the Flash Ready Light will light with blinking and the device does not emit the flash.
2).Once the Light Exit Window is close to the skin, the flash is continuously exposed for 8 seconds, the Flash Ready Light will be light with blinking and device stop emitting flash.
3)."Auto Emit Flash mode" is recommended for large area hair removal.
4)Ensure that the ENTIRE AREA receives treatment, but DO NOT overlap treatment pulses.

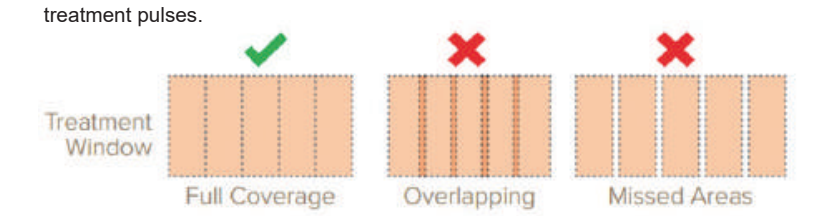

- **Mode switch**: During device working, take away device from the skin, press and hold the Flash Button for about 2 seconds, if there are Flash Ready Light lights with blinking, the device is switched into "Auto Emit Flash mode",press and hold the Flash Button for about 2 seconds, if there Flash Ready Light lighting on, thed evice is switched into "Manual Emit Flash mode".

4.2. Skin Test Patch

※For first-time users, we recommend you to test the device on the arm for reactions with following skin test patch:
a.Turn on the device, select the intensity level 1, press the Device probe on the skin and apply one flash.
b.Wait 24 hours and check your skin for any reaction such as discomfort or pain.
c. If the skin on the test site is normal (no discomfort or pain), you can continue to use it,if it is abnormal, please stop using it.
d.Increase the intensity by one level, and slide the device to the next area (do not flash multiple times on the same area). Test each intensity level according to above steps a)to c).Stop increasing the intensity level and stop the testing when the device causes any discomfort (or pain). Example: You can increase the intensity to level 2 and test it according to above steps a) to c) only when the device does not cause any discomfort (or pain) at level 1.

※After you test the skin, choose the intensity levels that did not cause a reaction on your skin.

※Wait for 24h each time after following the test patch to verify if your skin has an adverse reaction to the treatment. If there is no visible reaction, you can use the device.

4.3. Using Suggestions

※Before using the device you removed hairs by using a long-lasting removing method, such as plucking, waxing, etc., wait until hairs start growing again to use the device.

- **Treatment areas**
Suitable for the body parts: small areas such as underarm and facial hair below the chin line and large areas such as legs.
- **Treatment time**
According to hair growth cycle, it is recommended to use the IPL Hair Remova Device once every two weeks for the first 3-4 times and gradually reduce the use according to hairs condition.
- **Skin tone/hair color reference chart**
Please refer to the chart below before you start using the device to determine if your skin tone and hair color are suitable to use ("√" means the device is suitable for you; "X" means the device is not suitable for you).

Darker skin tones absorb more light easily causing skin irritation. Therefore, persons with darker skin tones are recommended to use a lower flash intensity light. For brown skin tone, please start from the lowest speed mode and adjust the speed setting according to your pain sensation.

SKIN Tone:
The product is suitable for the skin tone in Type I to Type IV. Please identify your skin tone and check the following table to see whether the product is applicable.

Skin tone table:

Skin type/color	View	Safety grade
Type I Pale white skin	✓	Applicable
Type II White skin	✓	Applicable
Type III Cream white skin	✓	Applicable
Type IV Moderate brown skin	✓	Applicable
Type V Dark brown skin	✗	Not Applicable
Type VI Deeply pigmented dark brown to darkest brown, black skin	✗	Not Applicable

HAIR COLOUR:
The IPL system is suitable for use on naturally black or brown hair. It may not be as effective on white, grey, blonde or red hair.

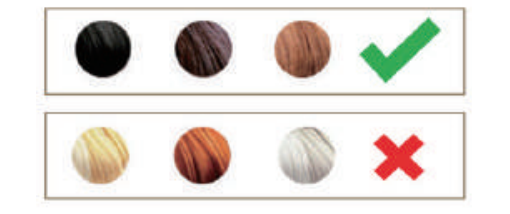

4.4. Using Steps

- Before you start using the device, use a razor or trimmer to shave all hairs on the surface of the skin (do not pluck or use chemical hair removal products) (figure 9), completely dry the skin and remove any oily substances (such as body fragrance, lotion, perfume, sunscreen, and other cosmetics).



Figure 9

- Connect power adaptor and main unit and then inserting the plug into a power socket.
- Press and hold the "On/Off/Level adjustment button" to turn on the device
- Select the appropriate flash intensity for your skin tone and hair color (for first-time users, use the lowest light intensity recommended and adjust it gradually).
- Wear protective goggles to avoid looking into the light (figure 10).



Figure 10

- Press the Device probe on the skin, ensuring the Device probe is fully in contact with the skin (Figure 11). Wait for a few secs, when the Flash Ready Light lights with blinking, press the Flash Button to apply the flash. You will feel a slight burning sensation (flash light energy being absorbed). If you want to reduce the burning sensation, adjust the treatment level.



Figure 11

- After use, turn off the device, unplug the power adapter, and clean the device.
Note:
1.The device is equipped with fan in the main unit which is used to cool the internal parts of the main unit during device working. When device is powered on, the fan begins working with a sound of the wind all the time until the device is powered off.
2.Clean the device according to chapter 6 of this manual after Unplugging the power Adapter for 20 minutes.
3.After cleaning, put the device and adaptor back to the packing box and storage it according to specified storage Conditions.

⚠ **Caution**
1.After using the device, DO NOT apply any fragrant skin care or cosmetic product on your skin.
2.DO NOT use deodorant immediately after using the device on the armpits. Waituntil the skin redness completely disappears to start using deodorant.
3.After each treatment, make sure your skin doesn't show any signs of redness after 24 hours.
4. Keep the treated area covered and away from direct sunlight two weeks after the treatment or use sunscreen (SPF30+) on the treated area.

5. Rare Side Effects

- **Burns,abnormal redness and swelling**
These reactions are very rare,They may be caused by using a high flash intensity.If these adverse reactions continue for 3 days or more, immediately consult a doctor. Only start the next treatment if the skin is clear of any problem, and make sure you use a lower flash intensity.
- **Skin discoloration**
Normal but very rare.When using the device, the skin may suffer from discoloration, this may happen because you are using a high-intensity flash When the discoloration disappears, reduce the flash intensity during the next treatments.If the skin discoloration does not disappear after two weeks. please consult a doctor.
- **Skin infections and inflammation**
Very rare. If the device is used in existing wounds and cuts (might happen when shaving the area)it can cause mentioned side effects.
- **Possible causes of excessive pain during and after the treatment**
You used the device on an area that was not shaved before you start the treatment; the flash intensity is too high for your skin tone and hair color; you used the device in the same exact area more than once, you used the device in an open wound; the area you are treating has any sort of inflammation or infection; you are using the device in areas with tattoos or sunburns.

6. Cleaning & Maintenance

6.1. Cleaning

After each use, clean this device following below tips:
Purpose: This device is for reuse to remove unwanted hair, you may clean the device surface since which can be contaminated during use with organic soil and microorganisms carried by human hands immediately after each use

Cleaning Agent: Use 70% isopropyl alcohol to wipe.
Method of Cleaning: To thoroughly clean the device, operate immediately after each use. Rub the device (including markings) such as the Light Exit Window, shell, button by hands without undue pressure with 70% isopropyl alcohol wiping for 15s and Light Exit Window for 3s.

Note:
1.Ensure that no liquid enters the interior of the device,
2.NEVER use abrasive cleaning agents, thinners or benzene for cleaning.
3.NEVER immerse the instrument in water or other cleaning liquids.
4. Wait 10 minutes after cleaning to allow the device to air-dry.

Visual Inspection: After cleaning, there should be no visible blotches and soil stains on the device under nature light, if there are still blotches and/or soil stains existed,repeat the cleaning steps mentioned above until there is no visible blotches and soil stains.

Disposing the device if there is corrosion, discoloration, pitting or cracked seals after cleaning, enquire about the options for environment-friendly and appropriate disposal.Take local regulations into account.
Reuse Life:999,99g Flashes

6.2. Maintenance

- The Light Exit Window is very delicate. it is very important to protect the Light Exit Window from dirt and damage. Do not touch or use tools to press it. It must be carefully protected.
- This device is not waterproof **DO NOT** immerse it or wash it under running water.
- **DO NOT** use steel wool, abrasive cleanser, chemicals or corrosive liquids to clean the device

7. Storage

DO NOT place or store the device for long periods in a hot or humid environment. Storage this device in following condition:

Storage environment	Temperature:-20~55 ℃ Relative humidity:5~95%,without condensation Atmospheric Pressure:70 kPa ~ 106 kPa

8. Recycling

At the end of its life, do not dispose of this device with the household waste. Please take this device to a local recycling point for proper. Proper disposaland recycling practices contribute to environmental protection.

9. Warranty & Support

- **Troubleshooting**

Problem	Possible Cause	Solution
Indication light is off	The power cable is not properly connected.	Check the connection of the power supply and adjust the cable.
	Only press "On/Off/Level adjustment button" , but not hold it.	Press and hold the "On/Off/ Level adjustment button" for about 2 seconds to turn on the device.
The device does not emit the flash	The power cable is not correctly connected	Check the connection of the power supply and adjust the cable
	The Device probe is not close enough to the skin.	Re-adjust the position of the Device Probe on your skin until the Flash Ready Light lights with blinking
During use the device has enter stand by mode.	The device power off automatically if no light is emitted within 5 minutes	Level adjustment button" for about 2 seconds to turn on the device
The device produces an odd smell.	The light exit window filter is dirty	press and hold the ""On/Off/ Carefully wipe the light exit window filter with 70% isopropyl alcohol.
	Hairs were not properly removed before the treatment The flash burns the hair causing an odd smell.	Before you start using the device, remove all hairs from the area you want to treat with a razor blade or trimmer
You feel pain when using the device.	The flash intensity is too high.	Verify the flash intensity and reduce it.
	The filter of the light exit window is damaged	Please stop using the device and contact your local dealer for assistance
	You are using the device in a non-applicable area.	Please read the instruction manual, warnings and prohibited use mentioned
After using the device, the treated area s hows signs of redness	Mild redness is a normal and harmless reaction to the hair removal	No need to take any action since it is a normal reaction.
The treatment results are not satisfying.	The flash intensity used is too low.	Adjust the flash intensity when using next time.
	The frequency is lower than recommended	In order to keep the skin smooth and without hairs, it's recommended to use the device once every two weeks. Treatment intervalsdepend on each person hair growth cycle. Do not use the device more than once every two weeks. Overusing may increase the risk of adverse skin reactions.
The treatment results are not satisfying.	Your skin tone and hair color are not suitable to use with this device	If your body hairs are blonde, red, gray white, or if your skin tone is very dark, do not use this device
Other problems.		Contact your local dealer.

Note: If the device still does not work properly after using the above solutions, please stop using the device and contact your local dealer.

10. Packing List

Main unit	1PCS	Power adapter	1PCS
Instruction book	1PCS	Safety goggles	1PCS
Glasses cloth	1PCS	Storage bag	1PCS

11. Specification Parameters

Device Name	Intense Pulsed Light (IPL)System
Model	PC-L10001
Dimension	139.5x83.3x48.3mm
Risk group	Exempt Group
Irradiation area	Light outlet: 4.0cm²
Adaptor Input	100-240 Va.c., 50/60Hz, 1.5A
IPL main part input	24 V.d.c., 2.0 A
Wavelength	510 ~ 1200nm
Max.Fluence	4.5J/cm²
Pulse duration	4 ~ 12ms
Output energy	5.6J~18J
Service life	999,999 flashes
Weight	254.5g
Operating environment	Temperature: 5 ~ 30°C Relative humidity: 20~90%, without condensation Atmospheric Pressure:70 kPa ~ 106 kPa
Storage and transportation environment	Temperature: -20 ~ 55°C Relative humidity:5~95%, without condensation Atmospheric Pressure:70 kPa ~ 106 kPa
Applied part	Type BF
No Sterilize requirement	
Not category AP / APG equipment	
Mode of operation: continuous	

Adaptor Technical specifications:

Item	Parameters
Model of adaptor	AK36WG-2400150DP
Input Voltage	100Vac~240Vac
Input Frequency	50Hz/60Hz
Service life for power adapte	10 years
Output voltage range	22.8 ~ 25.2Vdc
Output current range	0 ~ 2A
output power	≤36W
output over voltage	≤ 170% of output voltage
current-limiting protection	4.5-7.5A

12. Frequently Asked Questions

Q:The device power off automatically during use.
A: The device will power off automatically when the internal temperature of the device is too high, please restart device after 10 minutes.

Q: Must I shave hair before each use?
A: No. But you are advised to shave the hair when it is longer than 5mm.

Q: Why is my hair still growing after few Times of treatment? Why is it notfalling out immediately after treatment?
A: The Intense Pulsed Light (IPL) System is a home IPL hair removal device which Applies very gentle pulses of light to the hair root. it works step by step gradually first of all, the hair Goes into its resting phase- the hair you have falls out, and gradually your body grows less hair in that area, and finally, the hair stops growing back,it takes Time.

It is a permanent hair remover. Hairs cannot be removed permanently until you have used the device for one period. it can only repress hair Growth and slow down hair growing speed at the beginning. The hair enters the sleep state under continuous action.Thus, permanent hair removal effect is achieved.

Q: Why didn't I achieve the same effect as the others, or no effect at all?
A: People have different physiques, and the difference of hair thickness and treated parts can affect the effecting cycle. The using cycle is an average value, of which the specific time may be slightly different.

Q: Which level is suitable?
A: There is no unified standard of the suitable levels, it all depends on your skin tolerance, the darker the skin color, the lower the level should be used. And start choosing the suitable level from the lowest one. The higher the level is, the more obvious the treatment effect is and the shorter the Treatment time is.On the contrary, if you use a low level, the treating time will be extended accordingly. It is recommended to do local skin tests on the treated skin part before each hair removal, and then start treatment on large skin areas after, making sure that no skin discomfort occurs on the second day.

Q:Will it hurt?
A: During the hair removal process, light waves will generate heat when encounter hair melanins, causing slight pain.Due to the different skin sensitivity and pain tolerance of different individuals, the actual feelings are different. it is recommended to accelerate the level slowly from the lowest one according to your actual situation.

Q: How to shave? What kinds of hair should be shaved off?
A:Generally speaking, you should shave hair on the armpit parts, bikini parts, and legs before use.The method makes shaving easier.
1.Use shaving cream or mild shower gel to lubricate the shaving area
2.Or, apply a hot towel on the shaving area for a few minutes, and gently shave the hair immediately after removing the towel, which will make shaving easier.

Q:Why is there a smell of scorched hair after use?
A: That's because the hair is not completely shaved. While using the light waves will generate heat when encounter melanin, which causes the smells of scorched hair. And that is normal.

Q: I want to remove my hair quickly. Can I use the device every day?
A: It is not advised to use the device every day. Hair has a growth cycle, you can use it according to the normal cycle: Use once every two weeks during the first 3~4 times and gradually decrease the number of using times after the hair growth slows down.

13. Important information Regarding Electro Magnetic Compatibility(EMC)

⚠ **Warning**: Using cell phone or microwave oven, HF surgical equipment magnetic resonance imaging or other radio radiant equipment near this device may cause malfunction or lead to loss of essential performance

⚠ **Warning**: Use of this equipment adjacent to or stacked with other equipment should be avoided because it could result in improper operation. If such use is necessary, this equipment and the other equipment should be observed to verify that they are operating normally.

⚠ **Warning**: Use of adapter other than those specified or provided by the manufacturer of this equipment could result in increased electromagnetic emissions or decreased electromagnetic immunity of this equipment and result in improper operation.

⚠ **Warning**: Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of Intense Pulsed Light (IPL) System, including cables specified by the manufacturer, Otherwise, degradation of the performance of this equipment could result.